

Rec'd PCT/PTO 22 OCT 2004
PCT/GB 2003 / 002372



INVESTOR IN PEOPLE

The Patent Office
Concept House
Cardiff Road
Newport
South Wales
NP10 8QQ

PRIORITY DOCUMENT

SUBMITTED OR TRANSMITTED IN
COMPLIANCE WITH RULE 17.1(a) OR (b)

REC'D 15 AUG 2003

WIPO PCT

I, the undersigned, being an officer duly authorised in accordance with Section 74(1) and (4) of the Deregulation & Contracting Out Act 1994, to sign and issue certificates on behalf of the Comptroller-General, hereby certify that annexed hereto is a true copy of the documents as originally filed in connection with the patent application identified therein.

In accordance with the Patents (Companies Re-registration) Rules 1982, if a company named in this certificate and any accompanying documents has re-registered under the Companies Act 1980 with the same name as that with which it was registered immediately before re-registration save for the substitution as, or inclusion as, the last part of the name of the words "public limited company" or their equivalents in Welsh, references to the name of the company in this certificate and any accompanying documents shall be treated as references to the name with which it is so re-registered.

In accordance with the rules, the words "public limited company" may be replaced by p.l.c., plc, P.L.C. or PLC.

Re-registration under the Companies Act does not constitute a new legal entity but merely subjects the company to certain additional company law rules.

Signed

Dated 9 July 2003



The
Patent
Office

31MAY02 E722851-1 D00056
P01/7700 0.00-0212581.3

Request for grant of a patent

(See the notes on the back of this form. You can also get an explanatory leaflet from the Patent Office to help you fill in this form)

The Patent Office

Cardiff Road
Newport
South Wales
NP9 1RH

1. Your reference

MNM/P33178GB

2. Patent application number

(The Patent Office will fill in this part)

0212581.3

30 MAY 2002

3. Full name, address and postcode of the or of each applicant (underline all surnames)

IMPERIAL COLLEGE INNOVATIONS LTD
47 Prince's Gate
Exhibition Road
London SW7 2QA

Patents ADP number (if you know it)

If the applicant is a corporate body, give the country/state of its incorporation

England

7409436001

4. Title of the invention

MEDICAL ANALYSIS DEVICE

5. Name of your agent (if you have one)

"Address for service" in the United Kingdom to which all correspondence should be sent (including the postcode)

Kilburn & Strode
20 Red Lion Street
London
WC1R 4PJ

Patents ADP number (if you know it)

125001

6. If you are declaring priority from one or more earlier patent applications, give the country and the date of filing of the or of each of these earlier applications and (if you know it) the or each application number

Country

Priority application number
(if you know it)

Date of filing
(day / month / year)

7. If this application is divided or otherwise derived from an earlier UK application, give the number and the filing date of the earlier application

Number of earlier application

Date of filing
(day / month / year)

8. Is a statement of inventorship and of right to grant of a patent required in support of this request? (Answer 'Yes' if:


- a) any applicant named in part 3 is not an inventor, or
 - b) there is an inventor who is not named as an applicant, or
 - c) any named applicant is a corporate body.
- See note (d))

YES


Patents Form 1/77

9. Enter the number of sheets for any of the following items you are filing with this form. Do not count copies of the same document

Continuation sheets of this form

Description	12
Claim(s)	4
Abstract	1
Drawing(s)	7 + 7 

10. If you are also filing any of the following, state how many against each item.

Priority documents	0
Translations of priority documents	0
Statement of inventorship and right to grant of a patent (Patents Form 7/77)	0
Request for preliminary examination and search (Patents Form 9/77)	1 
Request for substantive examination (Patents Form 10/77)	0
Any other documents (please specify)	0

11. I/We request the grant of a patent on the basis of this application.

Signature



Date 30-5-2002

12. Name and daytime telephone number of person to contact in the United Kingdom

M N MAGGS
Tel: 020 7539 4200

Warning

After an application for a patent has been filed, the Comptroller of the Patent Office will consider whether publication or communication of the invention should be prohibited or restricted under Section 22 of the Patents Act 1977. You will be informed if it is necessary to prohibit or restrict your invention in this way. Furthermore, if you live in the United Kingdom, Section 23 of the Patents Act 1977 stops you from applying for a patent abroad without first getting written permission from the Patent Office unless an application has been filed at least 6 weeks beforehand in the United Kingdom for a patent for the same invention and either no direction prohibiting publication or communication has been given, or any such direction has been revoked.

Notes

- If you need help to fill in this form or you have any questions, please contact the Patent Office on 0645 500505.
- Write your answers in capital letters using black ink or you may type them.
- If there is not enough space for all the relevant details on any part of this form, please continue on a separate sheet of paper and write "see continuation sheet" in the relevant part(s). Any continuation sheet should be attached to this form.
- If you have answered 'Yes' Patents Form 7/77 will need to be filed.
- Once you have filled in the form you must remember to sign and date it.
- For details of the fee and ways to pay please contact the Patent Office.

MEDICAL ANALYSIS DEVICE

5 The present invention relates to a medical analysis device and to methods for fabricating and/or using such a device. It finds particular application in magnetic resonance spectroscopy or imaging, for instance for analysis associated with surgery.

10 Magnetic resonance imaging ("MRI") for medical diagnosis is well known. Typically, the entire patient or at least that part of the patient to be studied is placed with the main magnetic field of an MRI scanner's magnet. This very strong, homogeneous and static main magnetic field (e.g. 0.5 T) causes the nuclear spins within the patient to align themselves with and against the magnetic field, thereby creating a net magnetic moment in each volume. A transmit coil, typically surrounding the patient, is then used to transmit an
15 excitation pulse which flips the magnetic moment away from its equilibrium position. As the magnetization decays back to its equilibrium state the spins gyrate around the equilibrium axis and emit signal at the frequency of gyration. This radio frequency signal may be picked up by a receive coil. The frequency of gyration is given by the local magnetic field strength experienced by each
20 spin. This local magnetic field strength is dynamically altered using the scanner's gradients. These superimposed gradients, one in each of the x, y and z directions, typically work at audio frequencies and provide the frequency and phase encoding needed for image reconstruction.

25 In minimally-invasive MRI, a separate, small, receiving coil or antenna is used to receive the signal, instead of or in addition to the radio-frequency coils of the MRI apparatus itself. Such a coil may be placed either adjacent to the patient's skin or may be inserted by means of a probe into a patient's body cavity, for example into the colon.

MRI is increasingly used during surgical procedures, particularly where tumours or other soft tissue needs to be removed. The area of interest is imaged by the MRI scanner, as surgery proceeds, with both the tumour and the cutting instrument being visible on screen. It is important to remove tumours and their margins without cutting into the affected tissue. Current practice for tumour removal is to mark the tumour boundaries under image guidance (e.g. x-ray, MRI) using markers such as titanium wires, and then to cut around these markers. The result is a lump of tumour, which should have a margin (shell) of healthy tissue surrounding it. It is critical that no off-shoots are missed. Usually this is confirmed by checking that all the markers have been removed. Furthermore, the operative site is scanned to identify abnormal tissue left and the removed tissue is placed into a tumour container or resection jar and sent off to a laboratory for further analysis. At the laboratory, x-rays may be taken and frozen sections made.

There are a number of advantages for using MRI for soft tissue imaging. Firstly, the technique does not use ionising radiation. Secondly, no harmful contrast agents are needed. The technique is truly three-dimensional. However, the main advantage is the unrivalled soft-tissue differentiation. MRI may show tumours and tumour margins indistinguishable from healthy tissue in other imaging modality, the naked eye or even to palpation.

In practice, there are a number of problems however. In particular, x-ray analysis of the tumour is not particularly efficient since x-rays do not provide high quality images of soft tissue. Although it would be possible to provide improved images by placing the tumour into another MRI scanner at the laboratory, that would be expensive and would mean either purchasing another scanner to do the analysis or, alternatively, interrupting the routine of a scanner

that would normally be used for scanning patients. Because of the time currently taken to analyse the excised tumour, if any problem is found (for example if only part of the tumour has been excised) the patient typically needs to undergo a further surgical operation. That is clearly undesirable.

5

In a related use of magnetic resonance, there is also increasing interest in spectroscopy of tumours for tumour classification.

10

According to a first aspect of the present invention, there is provided a container for containing material to be analysed using magnetic resonance, the container including a receive coil for use in analysing material contained in the container.

15

Such a container can be placed within the magnetic field of a magnetic resonance scanner for use during surgery and material which has been removed from a patient can be placed in the container for imaging, during or immediately after a surgical operation, and preferably while it is still available to resume surgery on the patient.

20

Thus, using an embodiment of the present invention, when a tumour is removed it can be placed into the container, within the magnetic field of the MR scanner being used during surgery, allowing the tumour to be imaged there and then, in detail. There are several advantages of such an arrangement. Immediately after the surgical operation has been completed, the surgeon can

25

check whether a tumour has been excised cleanly, with a sufficient margin of healthy material around it. This can be done in the operating theatre, while the patient is still in the scanner and at very little additional cost.

The coil included in the container may also be adapted to act as a transmit coil for use in analysing material contained within the container. In such an arrangement, it may not be necessary that the container be placed in the transmit coil of the MR scanner being used during surgery since the container coil itself, acting in transmit mode might be used to create the necessary excitation pulse. Typically, the container will still be positioned within the main magnetic field and the gradients produced by the MR scanner, since the coil may provide an excitation pulse only without simultaneously being used as a receive coil. However, it would be possible for the coil to be used for both transmit and receive.

Preferably, the container is sealable; it may also have access points (e.g. rubber membranes) for biopsies.

Once the surgeon has finished, the container may be sent to the laboratory for x-rays and/or other analyses to be carried out in the normal way.

Preferably, the container is provided with a connector for connecting the receive coil, directly or indirectly, to an input of a magnetic resonance scanner. In this way, the container can be manufactured as a throw-away item, including just the container with its receive coil and the connector.

In more detail, receive coils for magnetic resonance may in use comprise an inductive part which is connected to circuitry such as matching and decoupling circuits. Preferably, only the inductive part is provided for the container. The more expensive circuitry can be provided as part of the input to a scanner, or as an adaptor for connecting the receive coil to a scanner. The use of an adaptor may be preferred since it supports the use of a single container design with multiple different scanners and/or field strengths. The adaptor can be scanner-

specific while the container is a standard item, without there being any need to manufacture a different container for each model of scanner. Containers may however be manufactured in a variety of shapes and sizes, according to application.

5

Thus in embodiments of the present invention the design can be flexible. It can use standardised scanner independent parts as throw away items. Expensive and specialised parts can all be multi-use.

- 10 Preferably, the receive coil is constructed as a volume coil so that material to be imaged can be placed inside the coil. This can provide improved resolution images. Such an arrangement might be particularly suitable for use with an "open" scanner in which patient scans can be carried out during surgical procedures, the surgeon often standing at least partially within the field of the scanner. . Open scanners bring huge advantages in guiding the surgeons but
15 current open MRI scanners have low to medium field strengths.

- The receive coil could be provided in different ways in relation to the container, and could indeed provide at least part of the containment. It could
20 be formed as part of the container body, or it may be added after the container itself has been manufactured. For example, the coil could be created by sputtering techniques, spraying, screen printing, painting etc. To avoid interfering with the scanner's magnetic field, the container, the receive coil and the connector for connecting the receive coil may be made entirely of non-ferromagnetic material.
25

According to a second aspect of the present invention, there is provided a scanner for use in analysis by magnetic resonance, the scanner having

detachably connected thereto a container comprising at least in part a receive coil for use in analysing material contained in the container.

5 The scanner may be an open scanner, provided with at least one transmit coil and at least one receive coil which can be arranged for use in imaging the area of a surgical procedure while it is being carried out. The container may be arranged so that it can be disposed in said area to enable analysis of material in the container by use of said at least one transmit coil, together with the receive coil comprised by the container. Alternatively or additionally, the receive coil
10 of the container may also be adapted to function as a transmit coil for use in analysis of material in the container.

An adaptor may be provided between the scanner and the container for adapting the detachable connection to meet requirements of the scanner and of
15 the receive coil of the container in said use in analysing material contained in the container.

According to a third aspect of the present invention, there is provided a method of analysing material by use of magnetic resonance, the method comprising the
20 steps of:

- i) generating a main magnetic field for use in analysing a body of material positioned in the field;
- ii) removing analysed material from said body of material;
- iii) placing the removed material in a container which includes a receive
25 coil, and placing the container in the magnetic field;
- iv) applying an excitation pulse to the removed material; and
- v) using the receive coil of the container in analysing the removed material.

Thus a method of analysis is provided in which some material is analysed twice, using MRI or MRS, once while in a body of material and once again after being removed therefrom.

- 5 The receive coil of the container might also be adapted to act as a transmit coil, in which case the excitation pulse used for analysis of the material while still in the body of material may be different from the excitation pulse used for analysis of the material after being removed therefrom. However, alternatively, the same excitation pulse could be used for analysis of the material while still in the body of material and after being removed therefrom. 10 The main magnetic field is preferably provided by the main magnet of an MRI scanner, with gradients being supplied by the scanner's gradient coils.

According to a fourth aspect of the present invention, there is provided a 15 method of analysing a sample material by use of magnetic resonance, the method comprising the steps of:

- i) placing the sample material in a sample container having a receive coil;
- ii) using a transmit coil external to the container to apply an excitation pulse to the sample material; and
- 20 iii) using the receive coil to analyse the sample material by use of magnetic resonance in response to the excitation pulse.

In this fourth aspect, embodiments of the present invention can provide a method of analysing material by placing the material in a container with a 25 receive coil and putting the container in a magnetic field generated independently and externally (e.g. by a MRI scanner). In such a method, there may be at least two receive coils, a first receive coil for use with the scanner in the normal way, in the absence of the container, and a second receive coil being the receive coil of the container.

In the above, reference is made to "analysis", "analysing" and the like. These are not intended to have any restricted special meaning and should be taken to encompass any operation that might be carried out using magnetic resonance
5 such as imaging, spectroscopy, or characterisation for example.

Embodiments of the present invention will now be described, by way of example only, with reference to the accompanying drawings in which:

Figure 1 shows a resection jar comprising a container according to an
10 embodiment of the present invention;

Figure 2 shows a receive coil for use with the resection jar of Figure 1;

Figure 3 shows a connector for connecting the receive coil of Figure 2 to a scanner input;

Figure 4 shows details of an inductively coupled example of the connector of
15 Figure 3;

Figure 5 shows details of a directly coupled example of the connector of Figure 3;

Figure 6 shows a circuit for use with the inductively coupled connector of Figure 4;

20 Figure 7 shows further coupling circuits; and

Figure 8 shows a cross section of the resection jar of Figure 1 with a sample positioned in the jar for imaging.

Referring to Figure 1, the resection jar can be a simple container 100 made of
25 clear material with an o-ring seal 105 and a threaded lid 110. In Figure 1(a), the container 100 is shown open and in cross section, exposing the thread 115 to attach the lid 110 to the body of the container 100. In Figure 1(b), the container 100 is shown closed and in cross section. In Figure 1(c), the

container 100 is shown closed and substantially in side view, in three dimensions.

5 The material of the container 100 is preferably transparent so that the position of a sample in it can be seen. Further, as mentioned above, the container and all its parts should be made entirely of non-ferromagnetic material. For example, the lid and body might be made of perspex or glass. The container may include access points, such as rubber-membrane-covered apertures (not shown) via which biopsies may be taken.

10

Referring to Figure 2, a solenoid coil 200 is wound onto the outside of the container 100 using for example adhesive copper tape. Solenoid coils are simple and give a good homogeneous magnetic field. The coil 200 could be used as a receive-only antenna, or as a transmit/receive antenna. As the scanner's main magnetic field needs to be perpendicular to the solenoid coil's axis, the configuration is well suited for scanners with horizontal magnetic fields and this includes most scanners. For scanners with vertical fields, the container 100 could either be turned onto its side, or a different configuration could be used.

20

Referring to Figure 3, it is necessary to connect the ends of the coil 200 to a connector 300 for connecting the container to a scanner for use. This can be done using enamelled copper wire 305 which is stripped at the contact points and soldered to the ends of the coil 200. It is then attached to the connector 300.

25

Referring to Figure 4, depending on the material of the container, the connector 300 could be glued to or screwed into the container 100. Figure 4 shows a version in which a screw 400 is used. It might be necessary to use several

screws. The ruggedness of the mounting would need to be adapted to suit the proposed use of the container. At the end of assembly, the entire container 100 is coated with an epoxy resin or other insulating, sealing and hardening varnish.

5 Referring to Figures 4 and 5, at least two different options exist for the design of the connector 300. The first option is to use inductive coupling, as shown in Figure 4. The second option is to use a direct connection, as shown in Figure 5.

10 Taking the first option, the connector 300 shown in Figure 4(a) provides the socket of a plug and socket arrangement. The plug component 405 is shown in Figure 4(b) and the two parts are shown coupled together and held by an O-ring 420 in Figure 4(c). The socket 300 and the plug component 405 each contain a
15 coaxial solenoid 410, 415 and their mutual inductance is used to transfer energy from the solenoid coil 200 towards the scanner. To put it another way, the solenoid 410 adds to or forms part of the coil inductance.

Taking the second option, as shown in Figure 5(a), the connector 300 again provides the socket of a plug and socket arrangement but this time it is
20 equipped with two pairs of resilient conductive blades 500. A plug component 405 for this form of the connector 300 is shown in Figure 5(b) and this is equipped with two conductive prongs 505 which can be pushed between the conductive blades 500 to complete the coupling, as shown in Figure 5(c). Each conductive prong 505 couples to a wire 305 such as is shown in Figure 3.

25

Both types of coupling are known per se, inductive and direct. Figures 6 and 7 show the circuitry suggested by each respectively. Such circuitry might be provided at an input to a scanner, or (preferably) as part of an adaptor for

connecting the container 100 to a scanner. The adaptor will typically be proximal to the container.

5 The circuits of Figures 6 and 7 are disclosed in "An inductively coupled, series-tuned NMR probe", *M. Decords, P. Blondet, H. Reutenauer, J.P. Albrand Journal of Magnetic Resonance 65, 100-109 (1985).*

10 Referring to Figure 6, for the inductively coupled circuit the container 100 will have to have a mounted capacitor C_s . Ideally it should be chosen to match a given field strength. However, it is also possible to use the same container for a range of field strengths, making more extensive provisions on the socket side. Figures 6(a) and 6(b) show equivalent circuits. At the socket side, we have control over L_p , r_p , C_m and M . Typically, r_p should be roughly zero, and M should be high. M , L_p and C_m may be adjusted to achieve matching.

15

Referring to Figure 7a, from the circuit point of view, the direct contact arrangement shown in Figure 5 is simpler. The container 100 need not have any components mounted other than the coil 200 and it may be used for all field strengths.

20

A decoupling scheme may need to be added if the coil 200 on the container 100 is to be used as receive only. This may be achieved using a DC bias on the coaxial cable to switch a diode at the input terminals of the matching section, as is shown in Figures 7(b) and 7(c).

25

Referring to Figure 8, material 800, 805 such as foam, preferably non-water-absorbing, may be inserted in the container 100 to ensure correct positioning of the sample 810 in the container 100.

Various design features may be preferred for use of the container 100. For instance, it may be preferred that the base of the container is made anti-slip and a label area might be provided on the outside. The entire container is preferably disposable and intended for single-use only. Alternatively, the
5 container may be made of suitable materials to allow sterilization and re-use.

In the above, attention is given to imaging of material, particularly to support surgical procedures. However, there may be other applications to which embodiments of the invention would be relevant. An example of one of these
10 is magnetic resonance spectroscopy of tumours for tumour classification.

CLAIMS:

1. A container for containing material to be analysed using magnetic resonance, the container including a receive coil for use in analysing material
5 contained in the container.
2. A container according to Claim 1, further including a connector for detachably connecting the receive coil, directly or via an adaptor, to an input of a magnetic resonance scanner.
10
3. A container according to Claim 2, wherein the connector provides an inductive coupling to the receive coil.
4. A container according to Claim 2, wherein the connector provides a
15 direct electrical contact to the receive coil.
5. A container according to any one of the preceding claims wherein the receive coil is also adapted for use as a transmit coil for use in analysing material contained in the container.
20
6. A container according to any one of the preceding claims wherein the container is sealable.
7. A container according to any one of the preceding claims wherein the
25 receive coil is constructed as a volume coil such that material to be analysed can be placed inside the coil.
8. A container according to any one of the preceding claims wherein the container is made of non-ferromagnetic material such that material contained in

the container can be analysed by use of an excitation pulse generated by use of at least one transmit coil external to the container.

5 9. A scanner for use in analysis by magnetic resonance, the scanner having detachably connected thereto a container including a receive coil for use in analysing material contained in the container.

10 10. A scanner according to Claim 9, said scanner being an open scanner, provided with at least one transmit coil and at least one receive coil arranged for use in imaging a three-dimensional space in which a surgical procedure can be at least partially carried out.

15 11. A scanner according to Claim 10 wherein the container is disposed in said space to enable analysis of material contained in the container by use of said at least one transmit coil, together with the receive coil of the container.

20 12. A scanner according to any one of Claims 9, 10 or 11 wherein the receive coil of the container is adapted to function additionally as a transmit coil for use in analysis of material contained in the container.

25 13. A scanner according to any one of Claims 9 to 12, the scanner being provided with an adaptor between the scanner and the container, for adapting the detachable connection to meet requirements of the scanner and of the receive coil of the container in said use in analysing material contained in the container.

14. A method of analysing material by use of magnetic resonance, the method comprising the steps of:

- i) generating a main magnetic field for use in analysing a body of material positioned in the field;
- ii) removing analysed material from said body of material;
- iii) placing the removed material in a container which includes a receive coil and placing the container in the magnetic field;
- iv) applying an excitation pulse to the removed material; and
- v) using the receive coil of the container in analysing the removed material.

15. A method according to Claim 14 wherein the receive coil of the container is adapted also to act as a transmit coil, for generating the excitation pulse.

16. A method according to claim 14 wherein the excitation pulse is generated by a transmit coil external to the container.

15

17. A method of analysing a sample material by use of magnetic resonance, the method comprising the steps of:

- i) placing the sample material in a sample container having a receive coil;
- ii) using a transmit coil external to the container to apply an excitation pulse to the sample material; and
- iii) using the receive coil to analyse the sample material by use of magnetic resonance in response to the excitation pulse.

20

18. A method as claimed in claim 17 including using apparatus external to the container to provide a main magnetic field within which the sample container is positioned during analysis.

25

19. A method as claimed in claim 17 including using apparatus external to the container to provide magnetic gradients within which the sample container is positioned during analysis.

ABSTRACT

5 A disposable container (100) which can be used to examine excised material during a surgical procedure is adapted for use with an open magnetic resonance scanner. The container (100) has a receive coil (200), provided in or on the body of the container (100), and can be connected (directly or indirectly) to an input of the scanner. During a surgical procedure which is monitored in known manner by magnetic resonance imaging, using the scanner, excised material such as a tumour can be placed in the container and imaged independently to
10 check for example that the tumour and a margin of healthy tissue has been removed. Conveniently, the container can be placed in the field of the open magnetic resonance scanner for imaging, using its receive coil. The container can also be used in magnetic resonance spectroscopy and tumour classification.

15

Figure 3b.

FIGURE 1

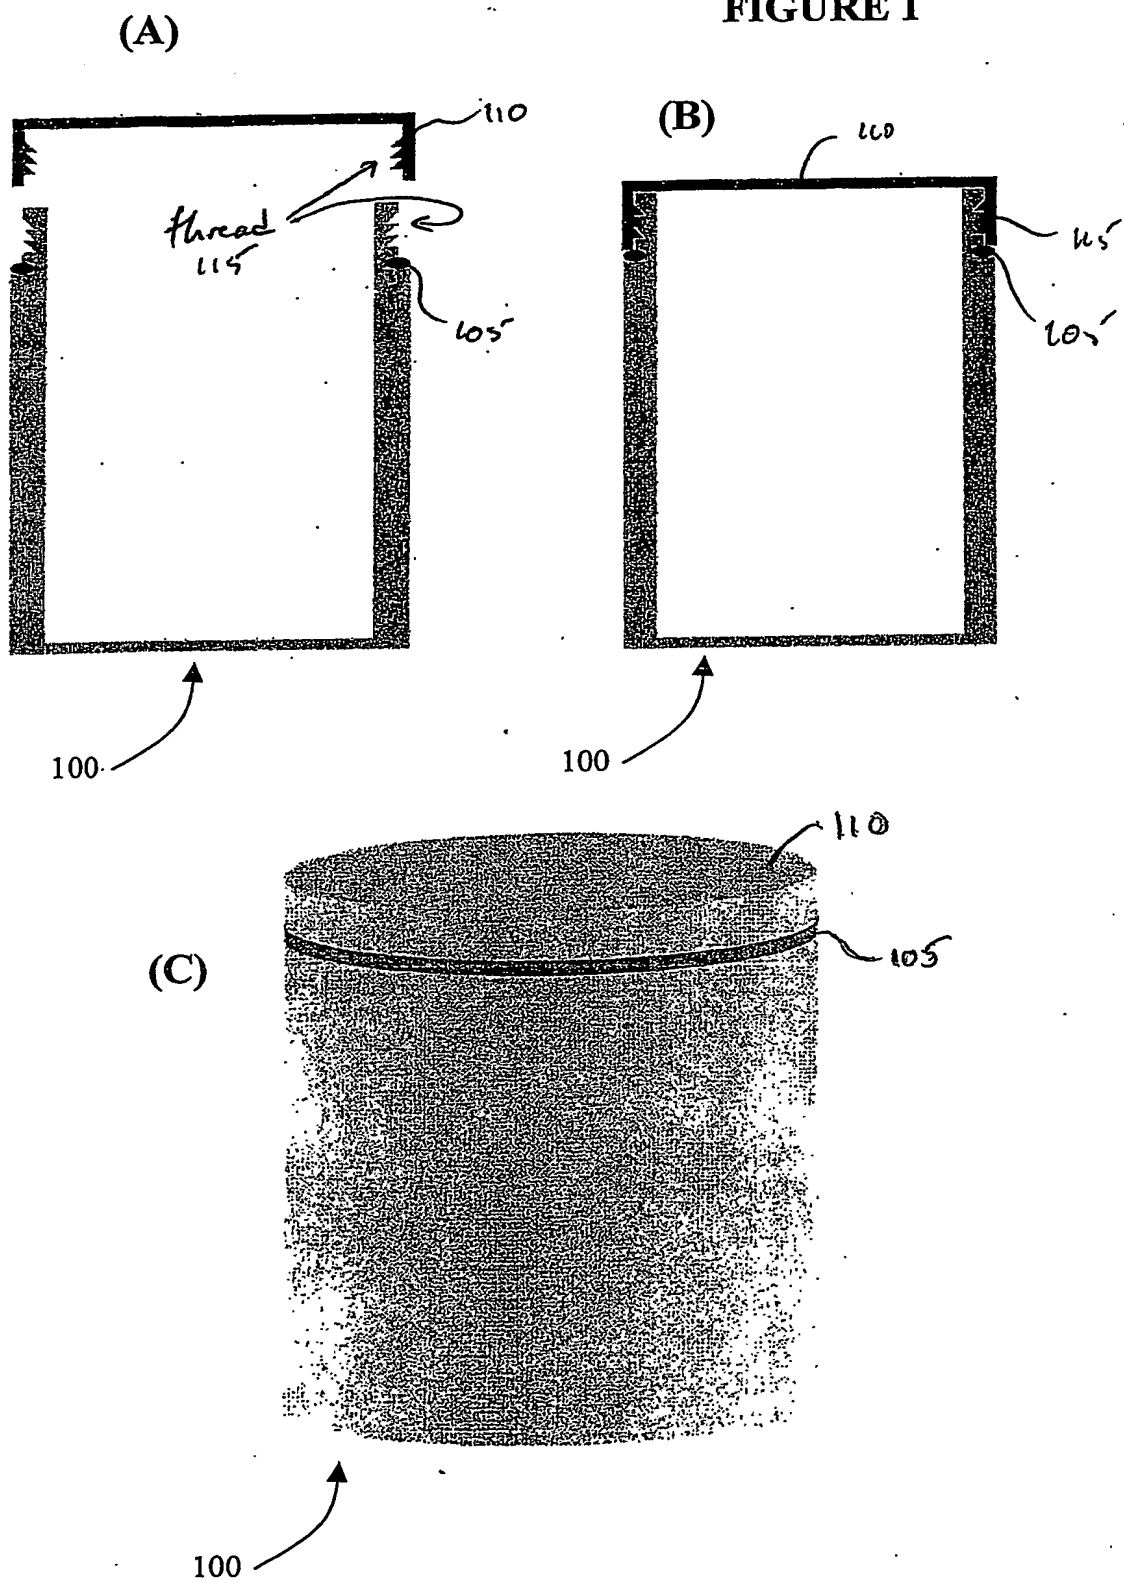
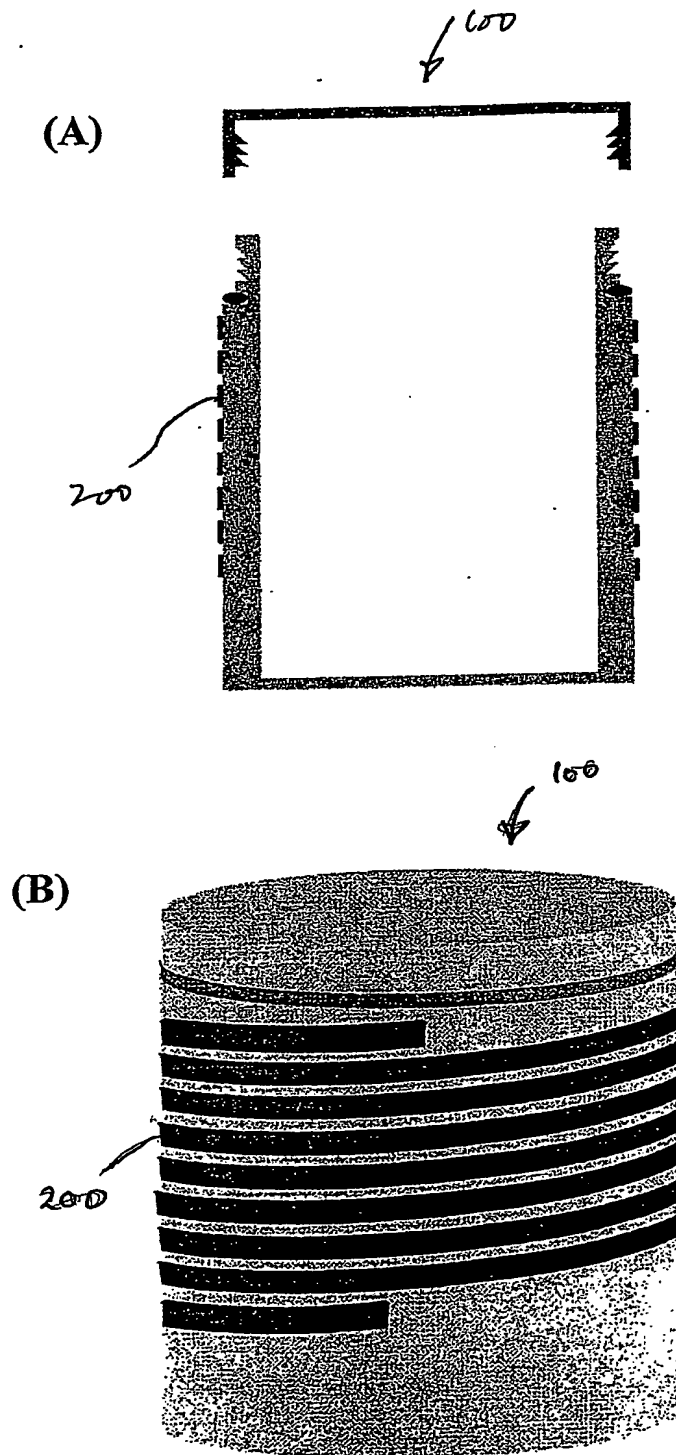


FIGURE 2



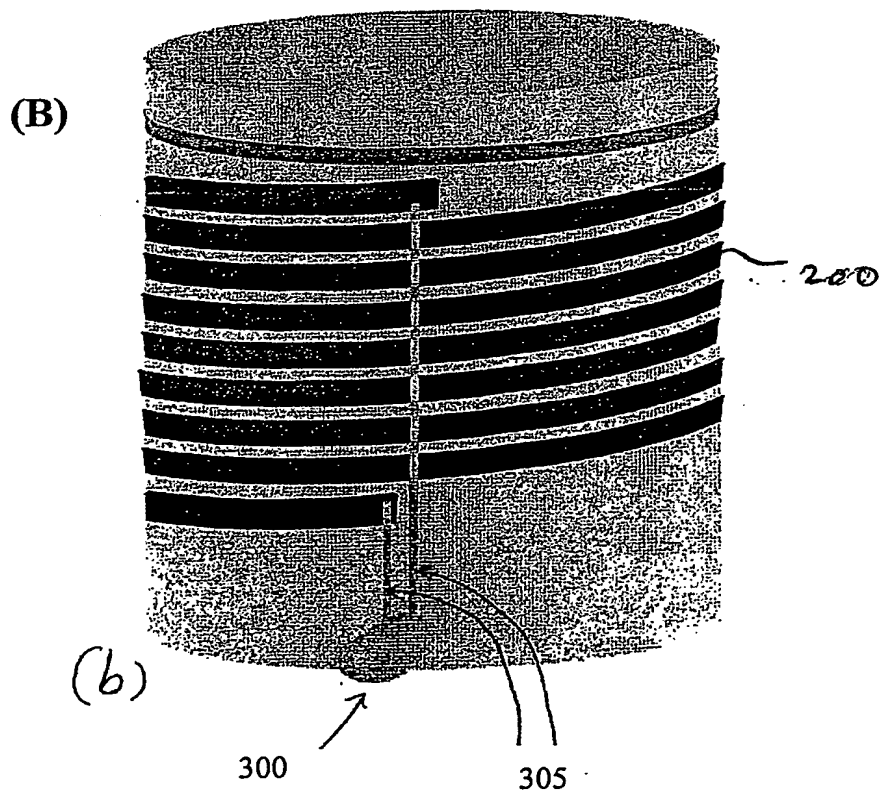
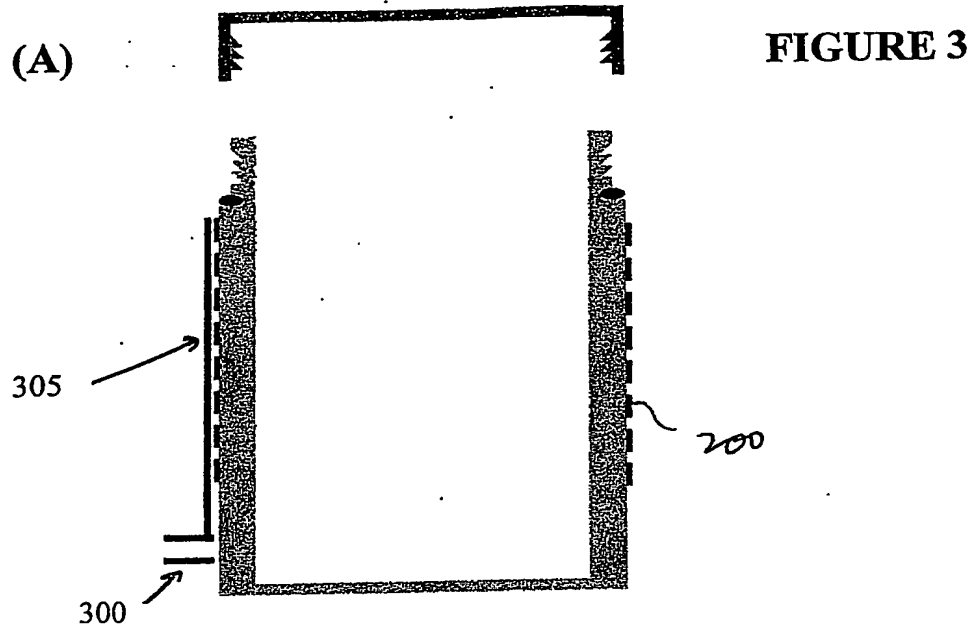


FIGURE 4

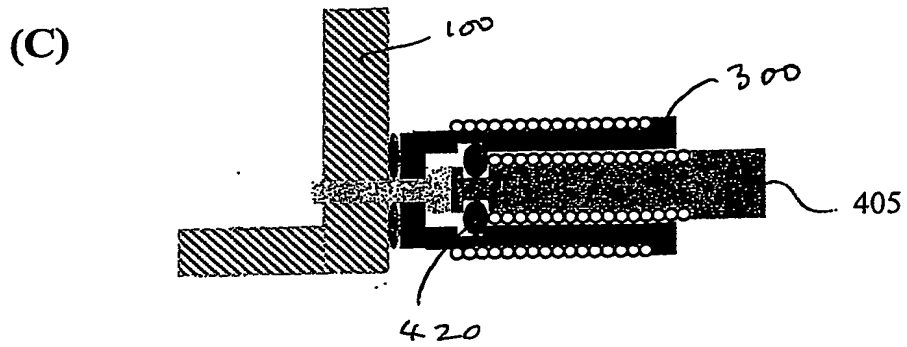
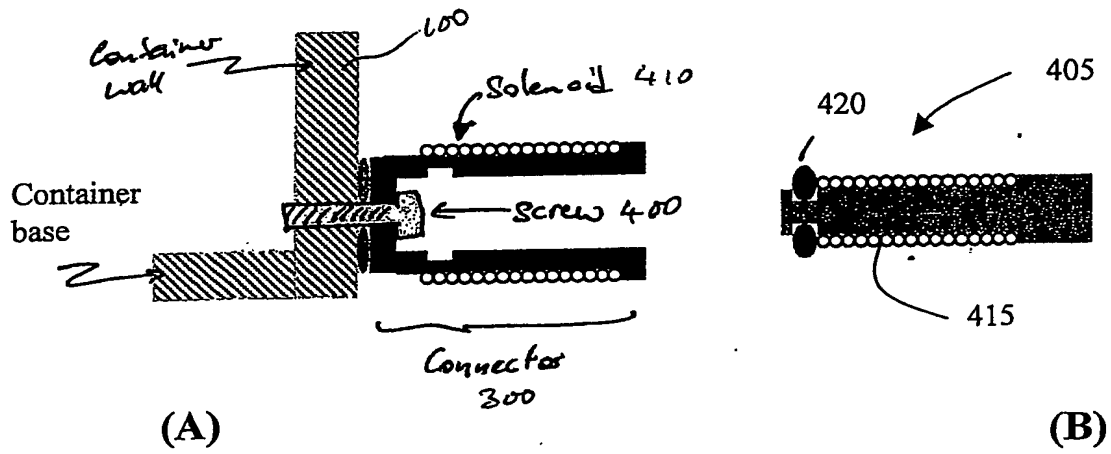


FIGURE 5




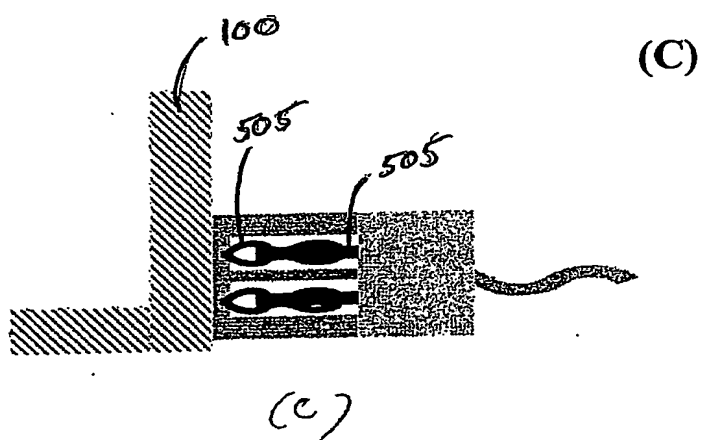


FIGURE 6

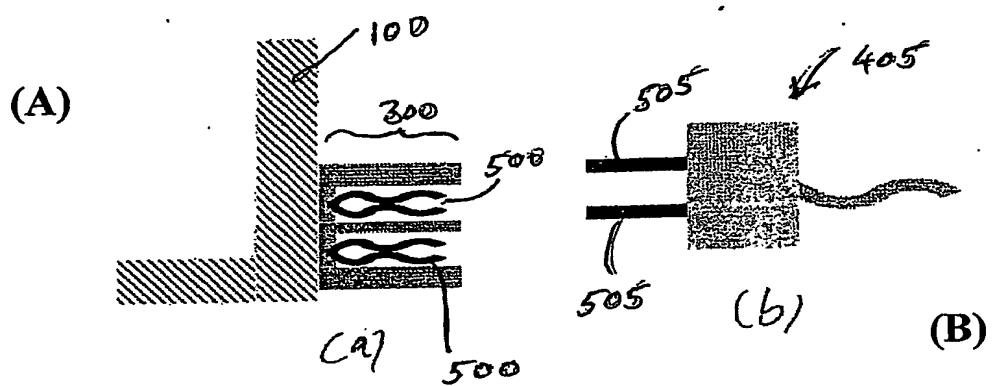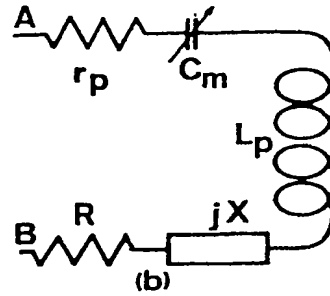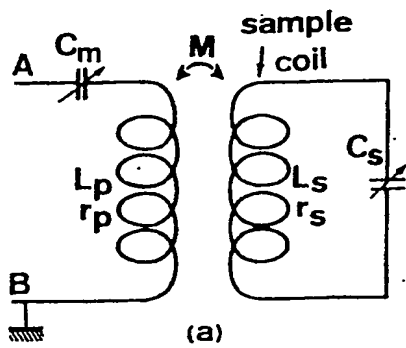

(B)

(A)

FIGURE 7(b)

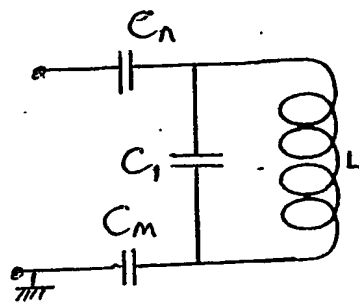


Figure 7(a).

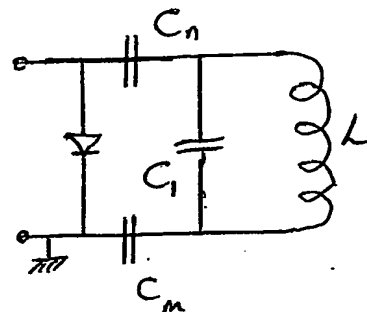
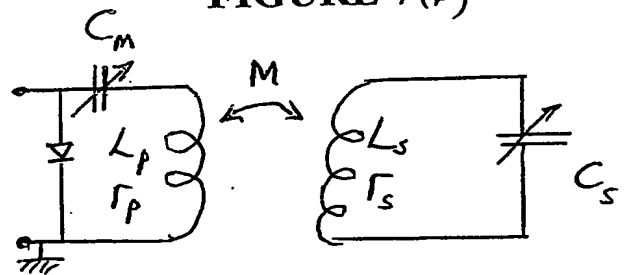


Figure 7(c)

717

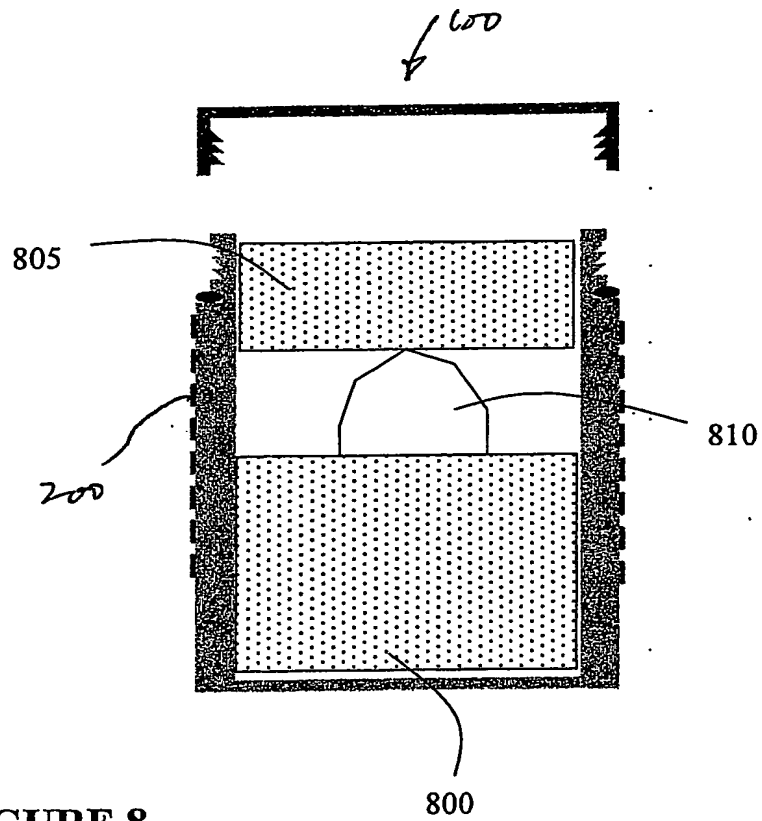


FIGURE 8

**This Page is Inserted by IFW Indexing and Scanning
Operations and is not part of the Official Record**

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

- ☐ **BLACK BORDERS**
- ☐ **IMAGE CUT OFF AT TOP, BOTTOM OR SIDES**
- ☐ **FADED TEXT OR DRAWING**
- ☐ **BLURRED OR ILLEGIBLE TEXT OR DRAWING**
- ☐ **SKEWED/SLANTED IMAGES**
- ☐ **COLOR OR BLACK AND WHITE PHOTOGRAPHS**
- ☐ **GRAY SCALE DOCUMENTS**
- ☐ **LINES OR MARKS ON ORIGINAL DOCUMENT**
- ☐ **REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY**
- ☐ **OTHER:** _____

IMAGES ARE BEST AVAILABLE COPY.

As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.